

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 662 001 BL

**Vol. flasks, 10 ml, NS 7, blue grad., A, conf. cert.**

**Batch:** 42-24


**Serial:**

**Measuring Nr.** 69537

**Batch size:**

1800

|                        |                   |
|------------------------|-------------------|
| <b>Volume:</b>         | <b>10,0000 ml</b> |
| <b>Tolerance:</b>      | $\pm 0,0250$ ml   |
| <b>Average value:</b>  | 10,0035 ml        |
| <b>Deviation:</b>      | 0,0041 ml         |
| <b>Precision (CV):</b> | 0,0408 %          |

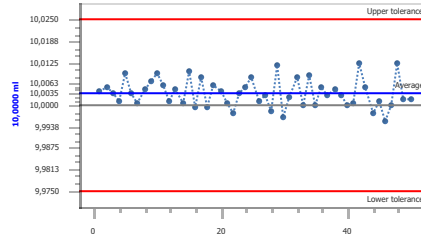

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

**Operator:**

4

**Date:**

21.10.2024

**Balance:**

Sartorius -  
MSE224S-0CE  
-DU

DE-M