

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 662 002 BL

Vol. flasks, 20 ml, NS 10, blue grad., A, conf. cert.

Batch: 43-24


Serial:

Measuring Nr. 71120

Batch size:

1197

Volume:	20,000 ml
Tolerance:	$\pm 0,0400$ ml
Average value:	20,0073 ml
Deviation:	0,0057 ml
Precision (CV):	0,0283 %

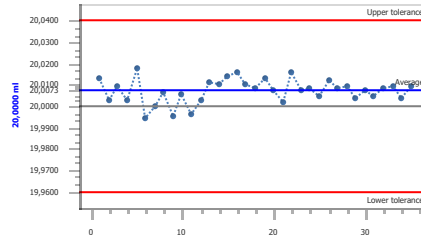

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 1042

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

09.12.2024

Balance:

Sartorius -
MSE224S-0CE
-DU

DE-M