

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 535 010 USP

Volumetric pipettes, 1 ml, USP, AS, conf. cert.

Batch: 42-24


Serial:

Measuring Nr. 70380

Batch size:

255

Volume:	1,0000 ml
Tolerance:	$\pm 0,0060$ ml
Average value:	0,9996 ml
Deviation:	0,0019 ml
Precision (CV):	0,1853 %

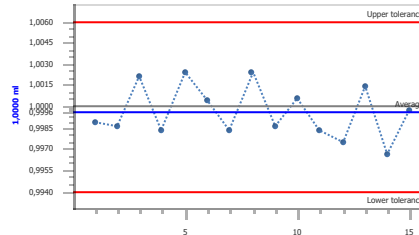

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 648

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	18.11.2024
Balance:	Sartorius - MSE224S-0CE -DU

DE-M